

# Assessment the photo-neutron contamination of IMRT and 3D-conformal techniques using thermo-luminescent dosimeter (TLD)

## Abstract

In radiation therapy with high-energy photon beams ( $E > 10$  MeV) neutrons are generated mainly in linac head thorough ( $\gamma, n$ ) interactions of photons with nuclei of high atomic number materials that constitute the linac head and the beam collimation system. These neutrons increase the out-of-field radiation dose of patients undergoing radiation therapy with high-energy photon beams. The purpose of the present work is to evaluate the dependence of photo-neutron production on field size, depth in phantom and distance from isocenter and also to calculate the equivalent neutron doses for PTV and OAR of IMRT and 3DCRT techniques using TLD (600/700). The results showed that; the photo-neutron production is decreased with increasing field size and distance from isocenter along patient couch while increased with depth in phantom up to  $d_{\max}$  and decreased gradually as increase depth in phantom. The measured equivalent neutron doses using 3DCRT for PTV and OAR were ranging from 0.027 to 0.39 mSv per photon Gy and for IMRT were 0.135 to 2.34 mSv per photon Gy.

Keywords: photo-neutrons, 3DCRT, IMRT, TLD.

## 1.Introduction

Radiotherapy means to convey a radiation dose (therapeutic dose) to kill all tumor cells which may cause harm to other sensitive organs, these organs called in the radiotherapy the organ at risk (OAR) [1]. According to the International Commission on Radiological Protection (ICRP), it is necessary to estimate all the sources of doses inside and outside the PTV to justify radiation doses to patients treated with radiotherapy (RT). Medical linear accelerator (Linac) with high-energy photon beams ( $>10$  MV) provide more deep penetration for greater depth dose, decreasing skin and peripheral doses due to less scatter than lower-energy beams. However these high-energy photons can also produce unwanted neutrons. The production of photo-neutrons mostly generated by the giant dipole resonance reactions ( $\gamma, n$ ) with high-Z material inside the head of the accelerators as the target, the flattening filter, collimator and multi-leaf collimator [2]. The dose from neutrons that produced during the therapy with high energy photon beams is un-accounted dose which may induce secondary cancer, the knowledge of the extra dose from neutrons in the vicinity of patient position is an important goal from the radiation protection point of view [3]. Three-dimensional conformal radiotherapy (3DCRT) is one of the radiotherapy treatment techniques that are based on 3D anatomic information and utilize dose distributions that acclimate as nearly as possible to the planning target volume (PTV) regarding adequate dose to the tumor and minimum dose as possible to the surrounding normal tissue. Intensity-modulated radiation therapy (IMRT) is another treatment technique of radiotherapy which provide non-uniform adequate dose to the patient from many different

angles of the treatment beam to optimize the composite dose distribution [4]. A thermoluminescent dosimeter (TLD) used to determine the equivalent dose of the neutron. Neutrons cannot produce direct ionization in a detector but they produce charged particles such as protons and alpha particles that thus cause ionization [5]. This work aims to assess the photo-neutron contamination for 15MV photon mode with different variables using TLD chips and to assess the photo-neutron contamination of IMRT and 3DCRT techniques using TLD chips.

## 2. Methods and materials

### 2.1 Thermoluminescence dosimeters (TLD Chips)

In the present study, the TLDs used were 6LiF: Mg, Ti (TLD600) which is sensitive to neutrons and 7LiF: Mg, Ti (TLD700) more sensitive to photons. These TLDs (TLD600 with 95.6% 6LiF and TLD700 with 99.9% 7LiF) are in the form of chips with dimension of 3.2 x 3.2 x 0.9 mm manufactured by Harshaw chemical company. The purpose of measuring the Element Correction Coefficient (ECC) for each chip to ensure that the entire population of TLDs were respond almost the same, all the chips irradiated with a single known dose 200 cGy using Siemens Linac 6 MV, the irradiations were performed with a field size of 10x10 cm<sup>2</sup> and Source to Surface Distance (SSD) of 100cm. The ECC is performed using the following equation:

$$ECC_n = \frac{\langle TLR \rangle}{TLR_n} \quad \text{eq.1}$$

Where the TLR is the average read-out of the TLD chips and TLR<sub>n</sub> is the read-out of the TLD number n [5].

This step has been repeated three times during this work.

Since TLD response is energy dependent, it is better to calibrate the TLD chips by the energy which is used in experiment [5]. Therefore, gamma calibration was performed by 15 MV photon beams.

#### 2.1.1 Gamma and Neutron calibration

The gamma calibration was done by two methods; Using 15MV Linac to irradiate all TLD chips, the chips were divided into 6 groups exposed to definite doses of (100, 130, 160, 190, 220, 250) cGy. The irradiations were performed in a RW3slab phantom 30x30x30cm<sup>3</sup> with a field size of 10x10cm<sup>2</sup> and max depth in phantom (d<sub>max</sub>=3) at **angle zero (°0)**. The other method of calibration presented in table 1. The TLDs were read out using PCL3 readout system (automatic reader) has been used for TLD measurements. After each use all the chips were annealed in a dedicated oven at 400°C for one hour followed by 100°C for two hours. Fig.1 shows the gamma calibration curve. Using 15MV Linac to irradiate all TLD chips as previous but using tungsten plates in front of the point of measurement serve as a moderator and to thermalize the fast neutron.

The neutron calibration was performed by A 5 Ci Am-241-Be source. All chips were placed at 1m distance from the source using 6 cm polyethylene as moderator in front of the chips. Data of calibration represented in table2.

Name	Type	Manufacturer	Cal. on
Cal. Source	$^{137}\text{Cs}$		
UNIDOS meter	App. Nr. 10001-10522	PTW, Freiburg	May/ 2017 (BIPM)
Ion chamber 30 cc	NE2530 (#424)	NE 2530	May/ 2017 (BIPM)

Table 1: Standard/ Reference/ Major used data of gamma calibration

Name	Type	Manufacturer	Cal. on	Results	St. Dev. 0.565
Cal. Source	Am-Be				Correction factor 0.066
Neutron monitor	NM2	NE., LTD.	Mar.2016 (PTB)		

Table 2: Standard/ Reference/ Major used data of neutron calibration

## 2.2 Assess the neutron contamination for 15MV photon mode with different variables.

In this step all the TLD chips (600 and 700) exposed to a single dose 200cGy with different variables as seen in the following figs (4, 5, 6, and 7). The equivalent dose  $H_T$  for neutron was calculated by the equation 2.

$$H_T = \sum W_r \times D_T \quad \text{eq. 2} \quad (\text{ref ICRP 60}).$$

Where:  $H_T$ = Equivalent dose (Sv),  $D_T$ = Absorbed Dose (Gy),  $W_r$  = Radiation weighting factor war calculated using ICRP-60 recommended formula (ICRP, 1991) [6].

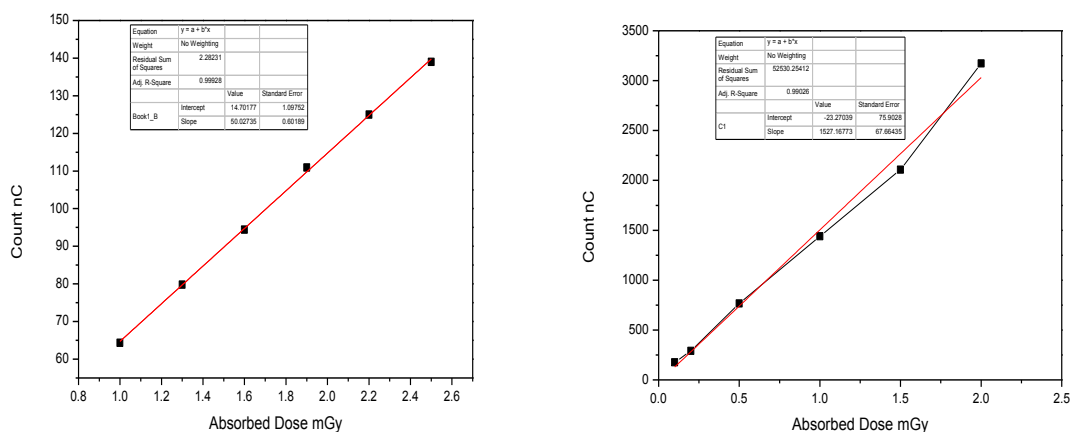


Fig. 1 the relation between gamma absorbed dose (mGy) and TLD reading (count in nC) with 15 MV photon irradiation on the left, and with ionization chamber on right side.

## 2.3 Treatment planning system

5 prostate cancer cases were selected in this study for patients completed their courses of radical radiotherapy to the prostate with high energy beam (15MV) Linear accelerator Siemens Oncor

impression, Germany, installed at Nasser Institute- Oncology Center. The OARs were bladder, rectum and femur. Using both 3DCRT and IMRT treatment plans. Once the plans were completed, there were copied from a patient onto the RW3 slab phantom. The phantom scanned firstly using Toshiba CT machine providing 4 multi-slices per rotation. The phantom images then transferred to XIO TPS (planning system) via the network. On the TPS, all fields of both treatment plans are transferred to the phantom, the total prescribed dose for each plan was 2.2Gy per 30 sessions to deliver total prescribed dose of 70Gy. A 5-field conventional 3D conformal plan has been used The gantry angles for the 5-field conventional 3D conformal were 0°, 45°, 90°, 270°, and 315°. A standard 5-field treatment was calculated for the slab phantom, as shown in (fig.2). The total numbers of Monitor Units (MU) for each angle were 77, 54, 70, 77, and 44 respectively irradiated per fraction resulting in a total dose to the PTV of 70 Gy. 7 radiation fields used in IMRT plan with angles 0, 51, 102, 153, 204, 255, and 302 (fig. 3). The total numbers of MUs for each angle were 52, 63, 87, 96, 53, 128, and 73 respectively. The plans were optimized to reduce the dose to the OARs to a minimum, while the dose to the PTV was maintained in accordance with the ICRU 83 Report [7].

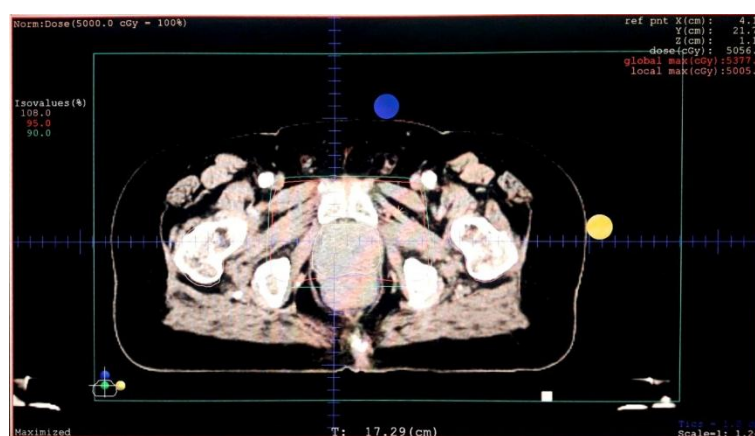


Fig.2 a standard 5-field treatment was calculated for the slab phantom.


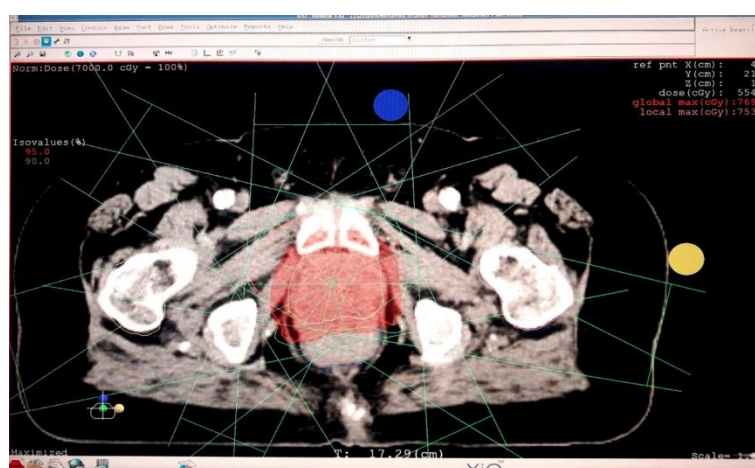


Fig. 3 shows the dose distribution of 7-field IMRT plan.


## 2.4 Results and Discussion

In the step of assessing photo-neutron production at different variables, the equivalent neutron doses in mSv per photon Gy is expressed with (mSv/Gy).


From fig.4 noticed that the equivalent neutron dose decreased with increase field sizes from 0.2 to 0.09 mSv/Gy with field size changed from  $2 \times 2 \text{ cm}^2$  to  $20 \times 20 \text{ cm}^2$ , this result has agreement with the previous published work [8] in which the equivalent neutron dose decreased with increase field sizes from 1 to 0.6 mSv/Gy using 18 MV Linac. The measured data in fig.5 showed that the largest equivalent neutron dose was at isocenter 0.15 mSv/Gy reached to 0.02 mSv/Gy at 100cm. this data correlated with the previous published works [9 -10]. In reference [9] the equivalent neutron dose is greater at the isocenter 1.35 mSv/Gy and decreases gradually with the distance away from the isocenter 0.0469 mSv/Gy at 75 cm, in reference [10] the equivalent neutron dose decreased from 3.5 mSv/Gy at the isocenter to 0.62 mSv/Gy at 100cm. the variation of equivalent neutron dose with depth in phantom showed in fig.6. The equivalent neutron dose increased reach to maximum at  $d_{\max} = 0.15 \text{ mSv/Gy}$  and decreased gradually as increased the depth in phantom reached to 0.07 mSv/Gy at 10cm depth in phantom. This result showed good agreement with the previous published work [11] in which the highest equivalent neutron dose was 0.67 using 18MV linac and decreased to 0.4 mSv/Gy at phantom's depth= 10cm.

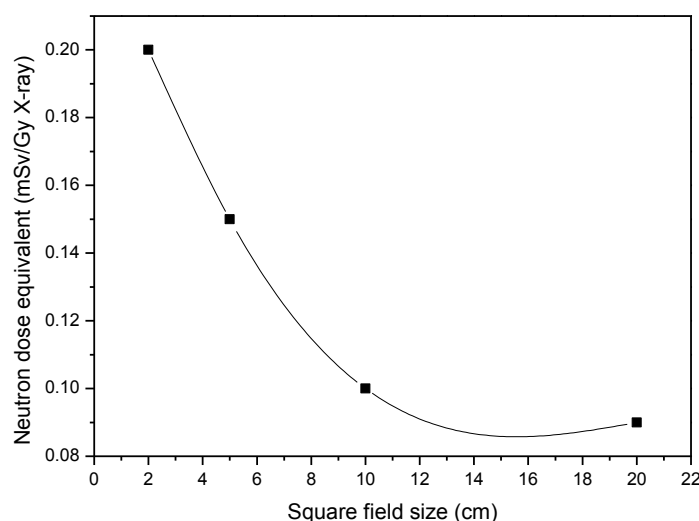

**Fig.4 Equivalent neutron doses** for different at the isocenter with SSD =100cm and zero angle using different field sizes ( $2 \times 2$ ,  $5 \times 5$ ,  $10 \times 10$ ,  $20 \times 20$ )  $\text{cm}^2$ .

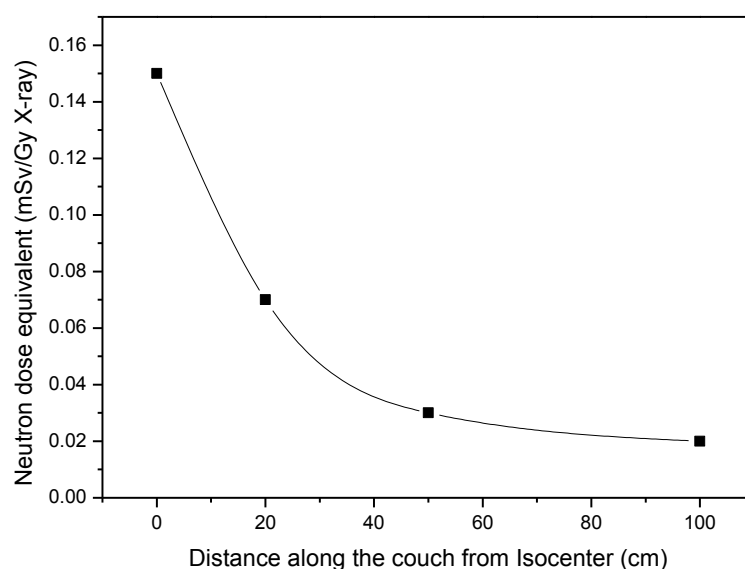

**Fig.5 Equivalent** neutron doses for different distances 4 selected positions on the patient couch of an 15 MV Siemens with FS (10x10) cm<sup>2</sup>, SSD = 100cm at zero angle using TLD chips.

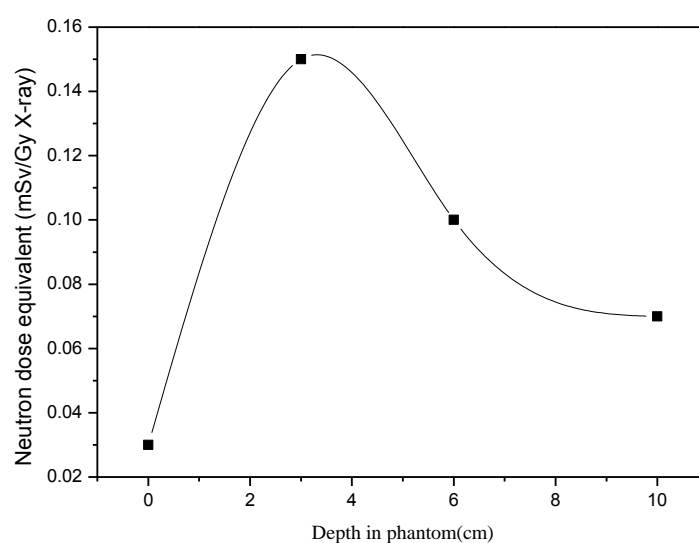

**Fig.6 Equivalent** neutron doses for 4 selected depths of 15 MV Simens Oncor with FS (10x10) cm<sup>2</sup>, zero angle at isocenter (depth=0) using TLD chips.

The measured equivalent neutron doses using 3DCRT for PTV and OAR were ranging from 0.027 to 0.39 mSv per photon Gy with average value 0.20 mSv per photon Gy (i.e. for 70 Gy treatment dose, the equivalent neutron dose was 1.89 to 27.3 mSv). For IMRT the measured equivalent neutron doses for PTV and OAR

were ranging from 0.135 to 2.34 mSv per photon Gy with average value 1.23 mSv per photon Gy (i.e. for 70 Gy treatment dose, the equivalent neutron dose was 9.45 to 163.8 mSv) as described in table2 and fig.7. These findings correlated with the published data [13], the neutron equivalent doses ranged between 0.5 and 3.6 mSv per photon Gy (i.e. for a 74 Gy treatment, the neutron equivalent dose range was from 37 to 263 mSv).

In 3DCRT the dose to bladder was nearly equal to the dose to the prostate that's because the location of the bladder is close to the prostate, while rectum received dose nearly equal to 40% from PTV dose. Rt. femur the dose was equal to 6% from PTV dose. In IMRT the doses at OARs were larger than doses with 3DCRT except for bladder the dose is larger than dose with IMRT that's due to the bladder in 3DCRT was located within the radiation field while in IMRT it was located partially in the field. These findings correlated with the published data [14].

Organ	3DCRT (mSv/Gy)	IMRT (mSv/Gy)
<b>Prostate (PTV)</b>	0.39±0.007	2.34±0.001
<b>Bladder (OAR)</b>	0.3±0.005	0.28±0.003
<b>Rectum (OAR)</b>	0.19±0.04	1.1±0.058
<b>Rt. Femur (OAR)</b>	0.027±0.01	0.135±0.02

Table3: Equivalent neutron doses for PTV and OAR using IMRT and 3D-CRT techniques.

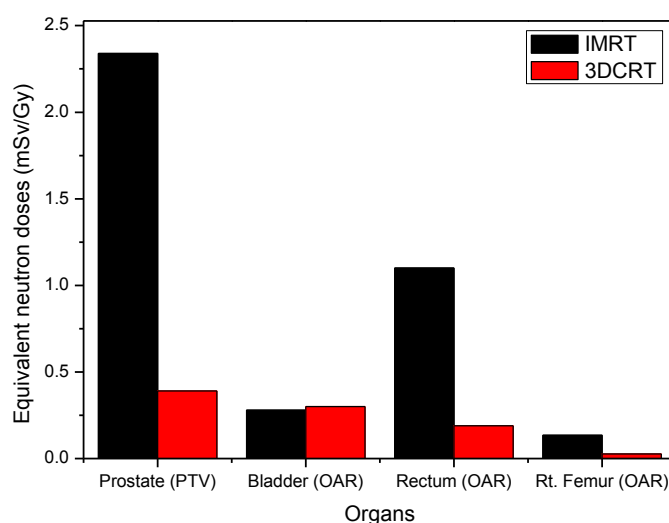


Fig.7 represents the equivalent neutron doses for PTV and OAR for IMRT and 3D-CRT techniques using TLD Chips.

## 2.5 conclusions

In conclusion: the photo-neutron production is varying with field size, gantry angle, depth in phantom and distance from isocenter along patient couch as described from the above figures. The contamination of therapeutic dose from neutron (neutron equivalent dose) delivered to the patient during the therapy is not negligible dose which reach to 2% with 3D-CRT and 39% with IMRT. As known IMRT improves target coverage and provide better OAR sparing comparing with 3DCRT. The use of IMRT resulted in worse OAR sparing than 3DCRT due to IMRT require more MUs to deliver the same dose to the PTV,



IMRT has more complex design with more scattering elements than 3DCRT so increases radiation risk induces secondary cancer, IMRT requires longer beam-on time than 3DCRT and during treatment with IMRT the field size changes which increase the production of photo-neutrons.

The fact that using high energy Linac produces photo-neutrons which constitute a significant part from the therapeutic dose to the PTV and OAR, also the TPS doesn't designed for neutron radiation then more research using Monte Carlo Simulation (MC) is required to measure the contamination of the therapeutic radiation dose with neutron when using high energy linac. Another study using GEANT-4 MC it will be prepared soon.

## References

- [1] Luther, W.B., Hans, P.H., Michael, M., 2006. Technical Basis of Radiation Therapy, 4<sup>th</sup> edition.
- [2] Dawn, S., Pala, R., Bakshi, A.K., Kinhikar, R.A. Joshi, K., Jamema, S.V., 2018. Evaluation of in-field neutron production for medical LINACs with and without flattening filter for various beam parameters - Experiment and Monte Carlo simulation. Radiation Measurements 04.005.
- [3] Yucel, H., Cobanbas, I., Kolbas, A., Yuksel, A.O., Kaya, V., 2015. Measurement of Photo-Neutron Dose From an 18-MV Medical Linac Using a Foil Activation Method in View of Radiation Protection of Patients. Nucl. Eng. Technol. 1–8.
- [4] Faiz, K. M., 2003. Physics of Radiation Therapy, 3rd edition.
- [5] Shagholi, N., Nedaie, H., Sadeghi, M., Shahvar, A., Darestani, H., Banaee, N., Mohammadi, K., 2014. Neutron dose evaluation of Elekta Linac at two energies (10 & 18 MV) by MCNP code and comparison with experimental measurements. Journal of advances in physics. 6 (1), 1006–1015.
- [6] ICRP, 1991. Recommendations of the International Commission on Radiological Protection. Ann. ICRP, 21(1/3).
- [7] ICRU, 2010. Prescribing recording and reporting intensity modulated photon beam therapy (IMRT). Washington: International Commission on Radiation Units and Measurements. (ICRU Report 83).
- [8] Mesbahi, A., Keshtkar, A., Mohammadi, E., Mohammad M., 2010. Effect of wedge filter and field size on photo-neutron dose equivalent for an 18MV photon beam of a medical linear accelerator. Applied Radiation and Isotopes (68), 84–89.



- [9] Sandipan, D., Rupali, P., Bakshi, A.K., Kinhikar, R.A., Kishore, J., Jamema, S.V., Abdul H., Palani, S. T., Deshpande, D.D., Datta, D., 2018. Evaluation of in-field neutron production for medical Linacs with and without flattening filter for various beam parameters - Experiment and Monte Carlo simulation. *Journal of Radiation Measurements* 04.005.
- [10] Bezoubiri, A., Bezoubiri, F., Badreddine, A., Mazrou, H., Lounis, Z., 2013. Monte Carlo estimation of photoneutrons spectra and dose equivalent around an 18 MV medical linear accelerator. *Radiat. Phys. Chem.* (2013), 07-013.
- [11] Yucel, H., Cobanbas, I., Kolbas, A., Yuksel, A.O., Kaya, V., 2015. Measurement of Photo-Neutron Dose From an 18-MV Medical Linac Using a Foil Activation Method in View of Radiation Protection of Patients. *Nucl. Eng. Technol.* 1–8.
- [12] Hussein, M., Aldridge, S., Guerrero U.T., Nisbet, A., 2012. The effect of 6 and 15MV on intensity-modulated radiation therapy prostate cancer treatment: plan evaluation, tumor control probability and normal tissue complication probability analysis, and the theoretical risk of secondary induced malignancies. *The British Journal of Radiology*, (85), 423–432
- [13] Kowalik, A., Jackowiak, W., Malicki, J., Skórska, M., Adamczyk, M., Konstanty, E., Piotrowski, T., Polaczek, K., 2017. Measurements of doses from photon beam irradiation and scattered neutrons in an anthropomorphic phantom model of prostate cancer: a comparison between 3DCRT, IMRT and tomotherapy. *62(1):29-35.*