

# **Helium-Neon Laser Effects on Human Whole Blood by Spectroscopy in Vitro Study**

## **ABSTRACT**

Low-power helium-neon laser recently has been used numerously in medical applications. FTIR and UV-Vis spectroscopic technique is employed to study the spectral differences in the serum of whole blood samples.

**Aims:** To study (He-Ne) laser ( $\lambda = 632\text{nm}$ , power= $2\text{mW}$ ) effect on human whole blood, after irradiated to different times from 10 min to 50 min.

**Study design:** Human Whole Blood Irradiated to (He-Ne) laser( $\lambda = 632\text{nm}$ , power= $2\text{mW}$ )

**Place and Duration of Study:** Institute of Laser, Sudan University of science and technology (SUST), Soba Hospital, Khartoum- Sudan, February 2018.

**Methodology:** Blood samples were collected from healthy volunteers; blood sample exposed to( H-N) laser and control compared; UV-Vis spectrophotometer and FTIR were used to study the effect of laser radiation.

**Results:** Absorption spectrum and FTIR spectra of whole blood are compared before and after He-Ne laser radiation shows, a significant decrease in intensity. FTIR spectrum of non exposed blood showed the peaks due to O-H (free group), C=O (amide I group), N=O (nitro group), and C-H (aromatic group). N-H (Amino acid (amide II) Laser radiation changes in transmittance in FTIR spectra for C=O group and O-H, N=O, the percentage of transmittance were increased. The most effects are found when whole blood irradiated to He-Ne laser radiation for 10 and 20 min and transmittance decreases for C-H, and N-H, due to denaturation of the protein.

**Conclusion:** Photodegradation of blood components due to absorption of laser radiation causes changes in the structure and conformational changes in the polypeptide and decrease intensity.

*Keywords: Laser, blood, UV-Vis, FTIR, spectroscopic*

## **1. INTRODUCTION**

Low-intensity helium-neon laser has been used extensively in medical applications.

Interaction of lasers with biological materials such as blood, skin, and tissues is important to be understood. The study of blood change by spectroscopic techniques can be used for understanding the biological nature of the disease, and also for the diagnosis of the disease [1, 2].

Photobiomodulations involves exposing tissues to low-level light. This type of therapy called Low-level laser therapy (LLLT), also known as cold laser therapy as

the power densities used produces no heating effect on the tissues. LLLT has a photochemical effect which means the light is absorbed and cause a chemical change. [3, 4, 5]

FTIR and UV-Vis spectroscopic technique are employed to study the spectral differences in the serum of normal blood samples[2], blood samples were irradiated in that study by He-Ne laser (Wavelength  $\lambda = 632.8$  nm, Power = 3mW). The FTIR spectra for irradiated blood samples showed significant changes [1]. He Ne laser ( $\lambda = 632$ nm, power=2mW) was used to irradiate human red blood cells and investigated by absorption spectrum, FTIR and fluorescence spectra of RBC. The absorption spectrum of RBC after exposure to He-Ne laser shows a significant decrease in absorbance. The FTIR spectrum of irradiated RBC clearly showed changes in transmittance [6]. Some rheological factors of the human blood, such as complete blood count (CBC) parameters and blood sedimentation rate (BSR) affected by low-level laser radiation (LLLR) laser blood biostimulation investigated the effect of LLLT on rheological parameters of human blood, they noticed a change in both viscosity and size of erythrocytes [7,8]. Human blood exposed to low-intensity He-Ne-laser radiation causes clearly defined changes in the IR and visible absorption spectra of the blood and erythrocytes. These spectral changes arise as a result of partial photodissociation of haemoglobin-ligand [9].

This paper investigates the effect of He-Ne laser (Wavelength  $\lambda = 632.8$  nm, Power = 2mW) with different exposure times using UV-Vis spectrophotometer and FTIR spectrometer.

## 2. MATERIAL AND METHODS

### 2.1 Samples Collection

Blood samples were taken from healthy volunteers; 3 ml of each volunteer by medical standard laboratory conditions and blood samples were saved in a tube to prevent from coagulation to (EDTA) and each sample was divided into two samples one sample was control and other exposed to the helium-neon laser with different exposure times.

### 2.2 Laser irradiated

Samples were exposed to a Helium-Neon laser beam, operating in continuous wave mode, as a radiation source (632.8 nm, 2 mW), for (10, 20, 30, 40 and 50) minutes The distance between the laser source and the samples was set to be 10 cm and the diameter of a laser spot was chosen to be 1.5 cm. To studied the effect of laser radiation were used UV-Vis spectrophotometer (Jasco-670) and Fourier Transform Infra Red Spectra (FTIR) were obtained used FTIR spectrophotometer (Shimadzu) for control, and He-Ne laser irradiated blood serum samples.


### 3. RESULTS AND DISCUSSION

59

60

61

#### 3.1 UV-Vis spectra

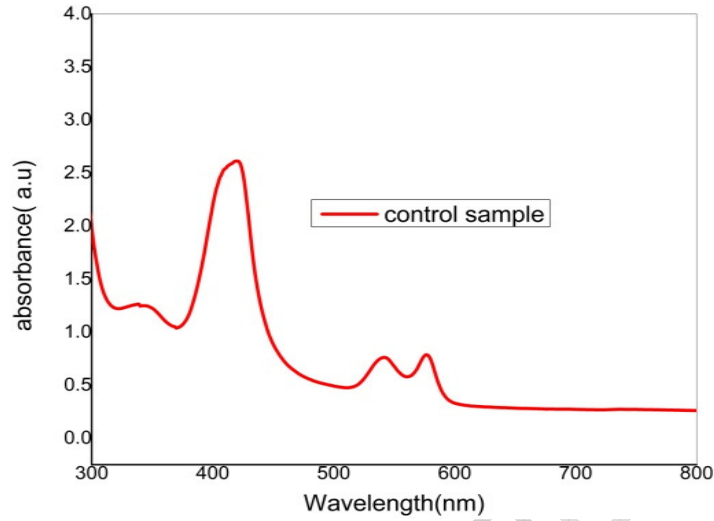

62

63


**Figure .1 Spectrum of non- irradiated blood sample (control).**

64

65

66

Figure 1 shows the spectrum of non- irradiated blood sample (control). This spectrum referred to non- irradiated blood sample which specified by peaks at (576.0, 542.0, 416.0 and 340.0) nm with intensities 0.793, 0.755, 2.604 and 1.253 respectively.

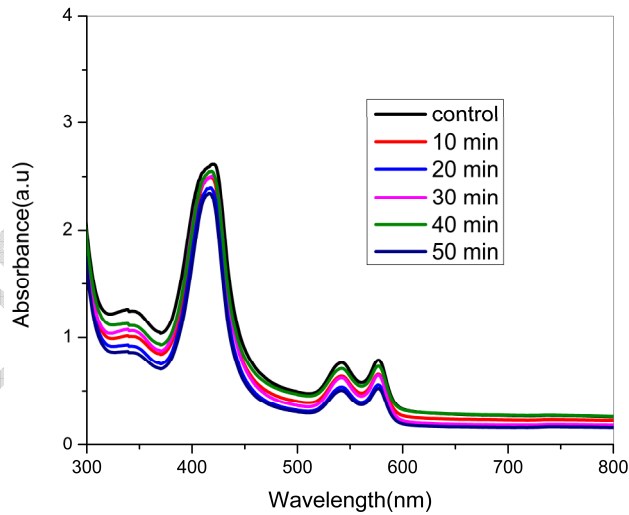

67

68

69

**Figure2. Relation between Absorbance (a) and wavelength ( $\lambda$ ) for whole blood before and after irradiated to (He-Ne) laser power 2 mW**

70

71

72

73

The absorption spectra of the whole blood recorded in the range of 300–800 nm Figure 2. Contain absorption bands with  $\lambda_{\text{max}} = 340, 416$  nm, a doublet band with  $\lambda_{\text{max}} = 542$  and 576 nm. We investigated only those changes in the absorption spectra of the whole blood exposed to the (He-Ne laser) radiation that was detected for all of the samples studied.

74

75

**Table.1 The intensity of normal and irradiated samples**

Wavelength (nm)	Absorbance (a.u.)					
	control	10 min	20 min	30 min	40 min	50 min
340	1.253	1.01	0.933	1.065	1.12	0.868
416	2.604	2.49	2.391	2.501	2.538	2.347
542	0.755	0.633	0.536	0.614	0.699	0.492
576	0.793	0.653	0.547	0.633	0.718	0.525

76 Different serum samples are analyzed quantitatively by calculating the intensities among the  
 77 absorption peaks which is show decrease intensity, all irradiated serum sample less than  
 78 control serum sample. These results indicate to that there is photodegradation happened to  
 79 the blood components. Laser radiation interacts with blood at the molecular level.  
 80 Hemoglobin is a blood photoreceptor that selectively absorbed.  
 81 Absorption intensity slightly decreases for all peaks at, due to increasing ligand  
 82 electronegativity [9].

83 In the UV-visible absorption spectrum of the irradiated blood, (figure.2 and table1) the  
 84 most intense absorption band at 416 nm, the light with this wavelength that strikes this  
 85 biological tissues will be highly absorbed. This phenomenon is the key for the desired effect  
 86 on the tissues [10]. Figure 2 compared the light absorption at 340nm, 414nm, 542nm and  
 87 576nm for different irradiation time. The minimum light absorption occurred at 50 minutes of  
 88 irradiation with the fewer intensities recorded. The concentration of absorbing centers is  
 89 decreasing. This fluctuation of light absorption is known as biphasic response. The  
 90 mechanism of LLLT at cellular level has been associated with the absorption of  
 91 monochromatic visible and near infrared radiation. Effective tissue penetration is maximized  
 92 at specific optical window [11].

### 93 3.2 FTIR spectra

94 **Table .2 FTIR spectral data (wave number, function group and transmission) for**  
 95 **normal blood control**

FTIR spectral data for normal blood (control )			
Sr. No	Wave number 1/cm	Group	% T
1	3444.63	O-H	0.48
2	1650.95	C=O	1.19
3	1548.73	N=O	6.36
4	1452.30	C-H	14.26

5	1317.29	N-H	15.3
6	1168.78	C-O	17.12

96

97 **Table .3 FTIR spectral data (wave number, function group and transmission) for**  
98 **irradiated blood sample blood control**


<b>FTIR spectrum of blood irradiated with he-ne laser for duration 10, 20, 30,40 and 50 min</b>				
Sr. No	Irradiated Time (minute)	Wave number 1/CM	Group	T%
1	10	3396.77	O-H	0.77
2		1650.96	C=O	1.78
3		1545.10	N=O	4.49
4		1450.73	C-H	15.20
5		1312.59	N-H	16.12
6		1161.74	C-O	18.70
7	20	3442.45	O-H	0.65
8		1651.63	C=O	1.68
9		1545.10	N=O	4.68
10		1451.01	C-H	11.43
11		1312.59	N-H	12.58
12		1161.74	C-O	13.76
13	30	3410.57	O-H	4.92
14		1651.63	C=O	6.50
15		1551.23	N=O	12.82

16	1451.01	C-H	22.14
17	1312.59	C-H / N-H	24.29
18	1167.96	C-O	26.31
19	3304.04	O-H	12.12
20	1645.41	C=O	13.21
21	1545.10	N=O	16.46
22	1447.23	C-H	25.43
23	1312.59	N-H	27.11
24	1161.74	C-O	28.50
25	3442.45	O-H	2.49
26	1651.63	N-H	6.46
27	1545.10	N=O	12.54
28	1451.01	C-H	22.28
29	1318.81	N-H	23.44
30	1167.96	C-O	25.59

99

100 An FTIR spectrum of whole blood in vitro without laser radiation is shown in (Figure) 3.  
 101 Table2. Shows the groups OH, C=O, N=O, C-O and C-H in the region between the wave  
 102 number  $4000\text{ cm}^{-1}$  to  $500\text{ cm}^{-1}$ . The most intense absorption band in proteins is the amide I

103 peak, which is observed at  $1650.95\text{ cm}^{-1}$ . Amide I is mainly associated with C=O symmetric  
 104 stretching and or C-O stretching vibrations. There are another very strong prominent amide  
 105 absorptions one at  $1545\text{ cm}^{-1}$  due to strong N-H in-plane bending and termed as an Amide II  
 106 band. The strong characteristic band at  $3295\text{ cm}^{-1}$  due to N-H symmetric stretching  
 107 confirmed the existence of amino acid group [2] The medium band at  $2873\text{ cm}^{-1}$  due to C-H  
 108 asymmetric and symmetric stretching of CH<sub>3</sub> group established the presence of lipids and  
 109 the medium bands at  $2854\text{ cm}^{-1}$  due to C-H symmetric stretching of CH<sub>2</sub> group established  
 110 the presence of lipids, fatty acids[12,13,15,15]. The FTIR spectra of blood showed clear  
 111 bands at  $1080$ , and  $12451\text{ cm}^{-1}$ , are composed of mononuclear cells containing nucleic acids  
 112 such as DNA and RNA. The nucleic acid components found in WBCs [9]. The bands at  $1170$   
 113  $\text{cm}^{-1}$  is associated with triglycerides of human blood. The band at  $2936\text{ cm}^{-1}$  is related to  
 114 platelets due to -C-H symmetric stretching of -CH<sub>2</sub>[16].  
 115 The whole blood sample is irradiated to He-Ne laser radiation for 10, 20, 30, and 40min. and  
 116 50 min duration respectively, figure (4 to 8) table 3. Shows the groups associated with  
 117 spectral peaks whole sample irradiated to He-Ne laser radiation for 10 min duration shows  
 118 an increase in transmittance for all groups except for C-H decreases due to the denaturation  
 119 of the protein. FTIR spectra of whole blood irradiated with He-Ne laser for 20 minute show  
 120 decreases in transmission for group, C-H, and N-H, to denaturation of protein i.e. it breaks  
 121 the polypeptide bonds due to conformational changes of proteins, but in 30, 40, and 50  
 122 minutes show an increase in transmittance for all groups is observed the separate  
 123 chromophore and auxochrome groups (C=O, N=O, C-H, N-H, C-O, O-H) show also  
 124 significant changes and indicates a significant increasing in their concentration. Laser  
 125 irradiation of blood causes changes in absorption band in stretching and bending Vibrations  
 126 of peptide group.

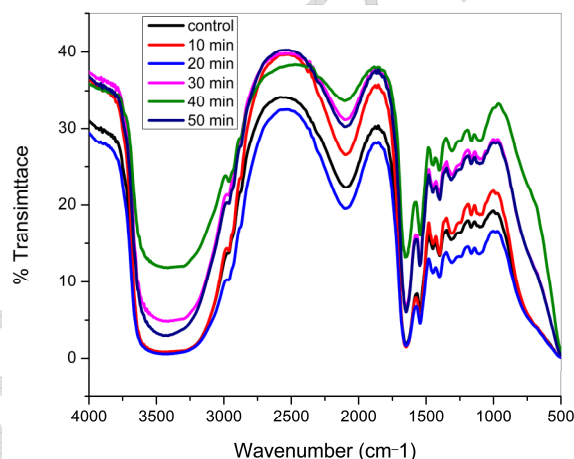

127  
 128 **Figure 3. FTIR spectra of irradiated blood by He-Ne laser for (0, 10, 20,30, 40 and 50)**  
 129 **minutes**

#### 131 132 **4. CONCLUSION**

133  
 134 This work had shown that laser radiation interacts with blood at the molecular level.  
 135 Hemoglobin is a blood photoreceptor that selectively absorbed He-Ne Laser beam with  
 136 output power 2mW, (632.8 nm). The absorption of laser beam by blood leads to partial  
 137 photodissociation. The results showed a decrease in intensity, all irradiated serum sample  
 138 intensity was less than control serum sample; this result indicates that there is  
 139 photodegradation happened to the blood components, this causes changes in the structure

140 and conformational changes in the polypeptide of N-H and CO and COO<sup>-</sup> groups in the  
141 regions 1500–1700 and 3000–3500 cm<sup>-1</sup> of the IR spectrum. Sample irradiated for 30, 40,  
142 and 50 minutes show an increase in transmittance for all groups is observed the separate  
143 chromophore and auxochrome groups (C=O, N=O, C-H, N-H, C-O, O-H) show also  
144 significant changes and indicates a significant increasing in their concentration.  
145

## 146 REFERENCES

- 147  
148 1-Ghadage VH, Kulkarni GR, Zaware BN. He-Ne laser irradiation of blood in vitro and FTIR  
149 spectral analysis. *Int J Chem Phys Sci*. 2015;4:148-53.  
150 2-Kanagathara N, Thirunavukkarasu M, Jeyanthi EC, Shenbagarajan P. FTIR and UV-  
151 Visible spectral study on normal blood samples. *IJPBS*. 2011;1(2):74-81.  
152 3- Fuad SS, Suardi N, Mustafa IS. In Vitro UV-Visible Spectroscopy Study of Yellow Laser  
153 Irradiation on Human Blood. In *Journal of Physics: Conference Series* 2018 Apr (Vol. 995,  
154 No. 1, p. 012053). IOP Publishing.  
155 4-Csele M. *Fundamentals of Light Sources and Lasers*, A Jhon Wiley and Sons. Inc.,  
156 Publication. New Jersey. 2004:360.  
157 5-Dais J. Low Level Laser Therapy Position Paper for the CMTBC: An Examination of the  
158 Safety, Effectiveness and Usage of Low Level Laser Therapy for the Treatment of  
159 Musculoskeletal Conditions. LLLT Position [Online]. 2009 Jul.  
160 6 - Ghadage VH, Kulkarni GR, Zaware BN. He-Ne laser irradiation of blood in vitro and FTIR  
161 spectral analysis. *Int J Chem Phys Sci*. 2015;4:148-53.  
162 7- Mi XQ, Chen JY, Liang ZJ, Zhou LW. In vitro effects of helium-neon laser irradiation on  
163 human blood: blood viscosity and deformability of erythrocytes. *Photomedicine and Laser*  
164 *Therapy*. 2004 Dec 1;22(6):477-82.  
165 8-Zahra Al Timimi MS, Jafri MZ. Photodynamic therapy and green laser blood therapy.  
166 *Global Journal of Medical Research*. 2011 Dec 23;11(5).  
167  
168 .9- Zaleskaya GA, Kalosha II. Effect of in vivo irradiation of blood by low-intensity emission  
169 from a He-Ne laser on molecular components of blood. *Journal of Applied Spectroscopy*.  
170 2009 Sep 1;76(5):720.  
171 .10-Mordehai J, Ramesh J, Huleihel M, Cohen Z, Kleiner O, Talyshinsky M, Erukhimovitch  
172 V, Cahana A, Salman A, Sahu RK, Guterman H. Studies on acute human infections using  
173 FTIR microspectroscopy and cluster analysis. *Biopolymers: Original Research on*  
174 *Biomolecules*. 2004 Mar;73(4):494-502.  
175 .11- Chung H, Dai T, Sharma SK, Huang YY, Carroll JD, Hamblin MR. The nuts and bolts of  
176 low-level laser (light) therapy. *Annals of biomedical engineering*. 2012 Feb 1;40(2):516-33.  
177 12- Robert Splinter, B. A. H. (2006). *An Introduction to Biomedical Optics*. Taylor & Francis  
178  
179  
180 13- Rathore S, Ali B. Effect of He-Ne Laser Radiation on Viscometric Behavior of Human  
181 Blood. *Journal of Chemical, Biological and Physical Sciences (JCBPS)*. 2013 May  
182 1;3(3):2124.



183  
184 14- Gunasekaran S, Uthra D. FTIR and UV-Visible spectral study on normal and jaundice  
185 blood samples. Asian Journal of Chemistry. 2008 Oct 1;20(7):5695.  
186  
187 15-Yu C, Irudayaraj J. Spectroscopic characterization of microorganisms by Fourier  
188 transform infrared microspectroscopy. Biopolymers: Original Research on Biomolecules.  
189 2005 Apr 15;77(6):368-77.  
190 16-Anders JJ, Borke RC, Woolery SK, Van De Merwe WP. Low power laser irradiation alters  
191 the rate of regeneration of the rat facial nerve. Lasers in surgery and medicine.  
192 1993;13(1):72-82.  
193 17-U. Vijaya Ushasree, Kaleem Ahmed Jaleeli and Adeel Ahmad A STUDY ON INFRARED  
194 SPECTROSCOPY OF HUMAN BLOOD International Journal of Science, Environment ISSN  
195 2278-3687 (O) and Technology, Vol. 5, No 3, 2016, 1189 – 1192  
196 .